	200TW Laser: Laser Safety Guidelines	Pág. 1 de 6
	Technological Area	Mar 2015
		Ed. 1 Rev. 2

200 TW LASER


Laser Safety Guidelines

- 1 Description of activity: CLPU laser facility
- 2 Laser types in use
- 3 Protocol
- 4 Laser Accidents
- 5 Laser alignment
- 6 Annexes
 - 6.1 Signature sheet

Before commencing work with Class 4 lasers, you must read this document, and sign the annex LSR-HRR that the Technological staff will give you to confirm this and your agreement to abide by the protocols contained herein.

The principal aim of this document is to outline the elements of good laser practice as they apply specifically to experiments currently being undertaken in the CLPU laser facility.

Redaction Head of Technological Area Technological Area Staff	Revision Managing Director Process Officer	Approval Director
--	---	---------------------------------

	200TW Laser: Laser Safety Guidelines	Pág. 2 de 6
	Technological Area	Mar 2015
		Ed. 1 Rev. 2

1. Description of activity: CLPU laser facility

In this laboratory various Class 4 pulsed and CW lasers are employed to investigate laser-matter interactions and nonlinear propagation as well as laser-characterization studies.

Depending on the experiment, several laser beams (they can have different wavelengths) are used. To facilitate this, laser pulses travel along well defined beam paths in the lab.


The laser system used in this lab is a 10 Hz, regeneratively amplified ~25 fs Ti:Sapphire laser with an additional multipass amplification up to 6 J in one of the outputs and 0.5 J in the other one. The mode-locked oscillator system is optically pumped by cw diode-pumped lasers while amplifiers are optically pumped by Nd:YAG diode lasers.

2. Laser types in use

Description	Laser type	Manufacturer	Pulse characteristics	Wavelengths	Pulse energies
200 TW laser system	Ti:Sapphire Flash lamp pumped	Amplitude	25fs, 10 Hz	760-840	6 J, 60 W
20 TW laser system	Ti:Sapphire Flash lamp pumped	Amplitude	25fs, 10 Hz	760-840	0.5 J, 5 W
Pulsed pump laser	Nd:YAG	Amplitude	10 ns	532	2 J, 20 W
Pulsed pump laser	Nd:YAG	Quantel	10 ns	532	150 mJ
Pulsed pump laser	Nd:YAG	Quantel	10 ns	532	30 mJ

As a general rule, all of these laser emissions are capable of causing severe eye damage (BLINDNESS) if viewed directly, or as a specular (i.e., mirror-like) reflection. Control measurements (careful planning, beam pipes, blocking of reflections, safety eyewear) must be taken to avoid this.

Authorized users of the above lasers are: supervisors, trained postdoctoral fellows students (compulsory with a supervisor or trained postdoctoral fellow's help), laser technicians.


	200TW Laser: Laser Safety Guidelines	Pág. 3 de 6
	Technological Area	Mar 2015
		Ed. 1 Rev. 2

3. Protocol

- Installation or changes must be discussed with a supervisor prior to operation of Class 4 laser systems.
- In the case of **any change or problem related to the laser beam**, the **200TW Laser Supervisor (LS)** must be consulted (cmendez@clpu.es).
- Laser beam paths and associated optics must be planned together with the lab **Coordinator** (japinaniz@clpu.es) or the **200TW Laser Supervisor (LS)** to minimize the possibility of stray reflections.
- Termination of each main laser beam must be planned also with lab supervisors or **Lab Coordinator (LC)**.
- Provision of suitable laser safety eyewear must be addressed.
- When starting the experiment, the **200TW Laser Supervisor (LS)**¹ will be responsible for activating or deactivating the **laser warning signs** in the display devoted to this whenever the laser is turned on and off.
- The **Experiment Supervisor (XS)**² will be responsible for activating or deactivating the **Experimental Area warning signs** in the display devoted to this whenever the status of the **Experimental Area** changes.
- All new laser users or visitors must receive an orientation to the laser use area by an authorized laser user.
- Alignment may be carried out by authorized persons, no one else may be present in the vicinity during this procedure and watches, bracelets and other reflective jewelry should be removed.
- Check stray reflection for every element you put in the beam path.
- Suitable beam blocks must be installed to block these stray reflections.
- If possible, install beam pipes to cover longer runs of laser beam.
- Under no circumstances must direct viewing of the laser beam be attempted even if the beam has been attenuated. There must be no exceptions to this (obvious!) rule.
- All optics must be checked for damage, and stability of optics mounts verified.
- Try to align with the lowest possible laser energy at which it is possible to visualize the laser beam in an appropriate fashion. The method of visualization is dependent on the wavelength: for UV or visible light, the beam can be viewed on a fluorescent card. An invisible infrared beam may be visualized using CCDs, heat sensitive papers or an IR viewer.
- Remember that lone working is inherently more hazardous than normal procedures and should only be undertaken when there is no alternative and only if it is safe to do so.
- Use proper safety methods when working with high voltage (contact the **lab supervisors** or **Lab Coordinator (LC)**, don't wear any jewelry, wear rubber bottom shoes, set up your work area away from possible grounds, and don't work alone).

¹ Or person authorized by the LS

² Or person authorized by the XS

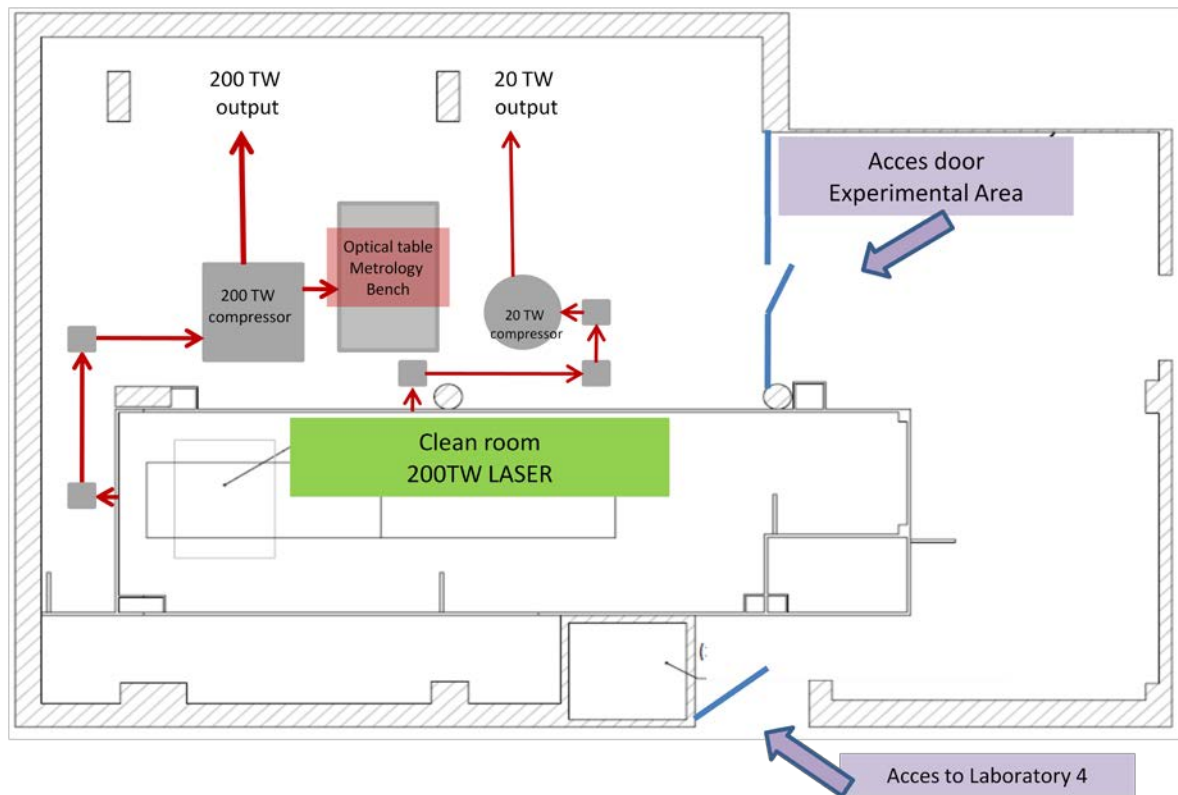


Sketch of 200TW laser beam lines

4. Laser accidents

Some common unsafe practices that are cause of preventable accidents are:

- Not wearing protective eyewear or using a wrong one during alignment/working procedures.
- Misaligned optics and upwardly directed beams- pay particular attention to periscopes, and reflections from windows and beam splitters/combiners.
- Improper methods of handling high voltage.
- Lack of protection from non-beam hazards.
- Failure to follow safety protocols.
- Bypassing interlocks and laser housing.
- Insertion of reflective materials into beam paths.
- Lack of pre-planning.
- Operating unfamiliar equipment without supervision.

	200TW Laser: Laser Safety Guidelines	Pág. 5 de 6
	Technological Area	Mar 2015
		Ed. 1 Rev. 2

5. Laser alignment

It has been reported that some sixty percent of laser accidents in research settings occur during the alignment process.

Laser alignment guidelines to help prevent accidents should include:

- Restricted access.
- Laser protective eyewear.
- Class 4 laser users must have received appropriate training and instruction.
- The individual who moves or places an optical component on an optical table is responsible for identifying and terminating each and every stray beam coming from that component.
- Watches and reflective jewellery should be taken off before any alignment activities begin.
- Beam blocks must be secured.
- Check the stability and rigidity of all optical mounts.
- When the beam is direct out of the horizontal plane, it must be clearly identified.
- The lowest possible/practical power must be used during alignments.
- When possible, a coarse alignment should be performed with a HeNe or cw diode alignment laser.

